

Figure 1 shows recommended adjustments from inversion of manual crossovers.

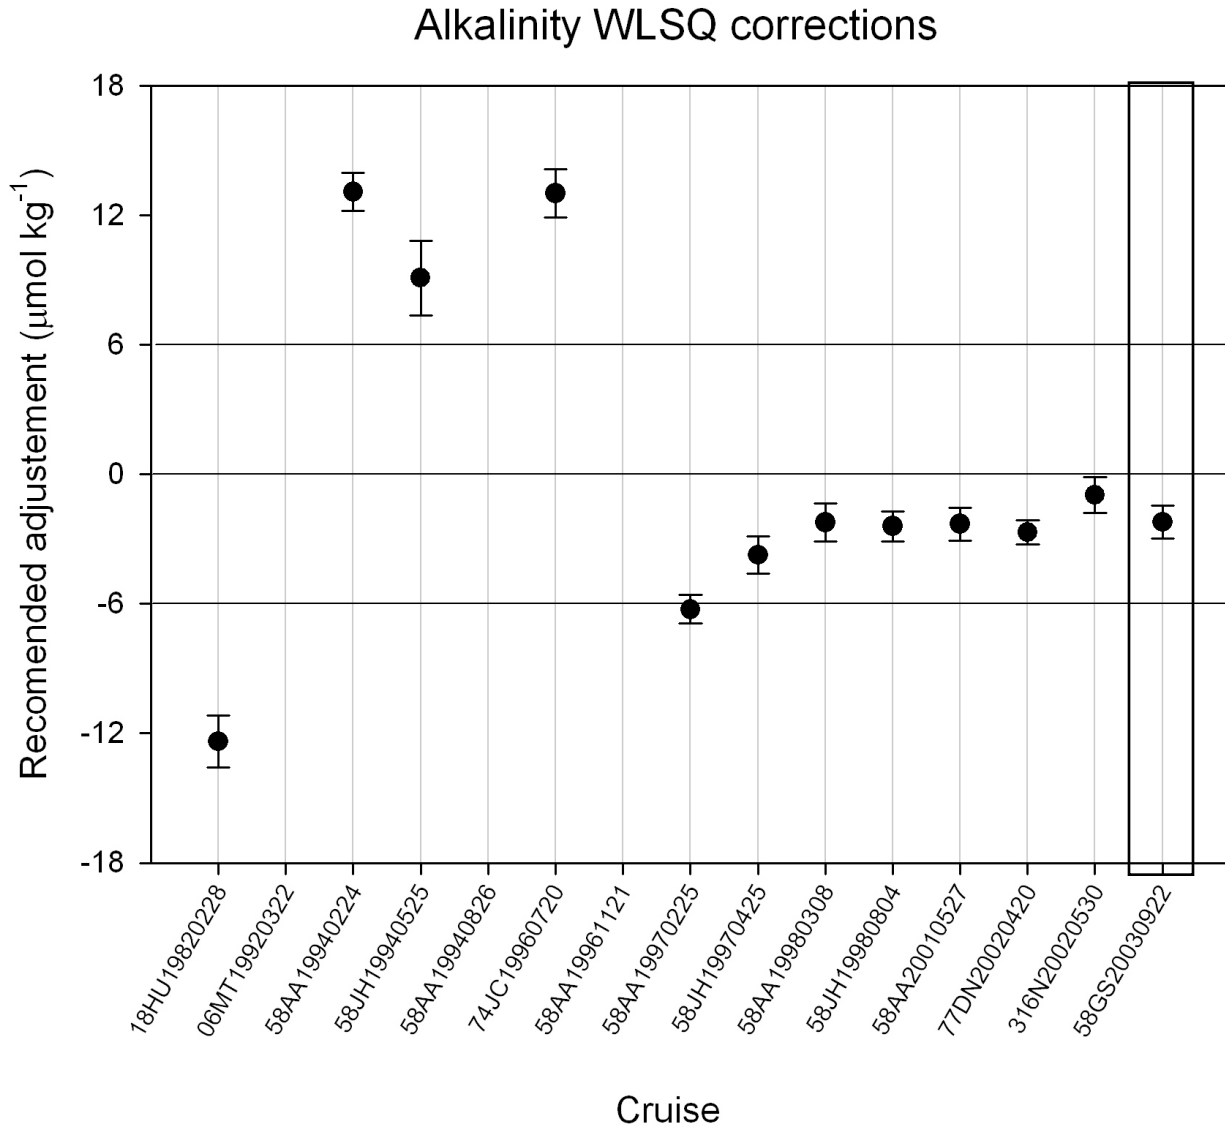


Figure 1: Recommended adjustments from WLSQ inversion of manual crossovers. Values are all in $\mu\text{mol kg}^{-1}$. Cut off for applying alkalinity correction is $6 \mu\text{mol kg}^{-1}$ as indicated with the lines in the figure.